
MT 2701	for RS 232
MT 2702	for RS 485
MT 2703	for TTY, Current Loop

Digitale Displays

with serial Input

Manual



ERMA

Electronic GmbH

Warranty

For delivered products our "Allgemeine Lieferungs- und Zahlungsbedingungen" are effective. In no event ERMA-Electronic or its suppliers shall be liable for any other damages whatsoever (including, without limitation, damages for loss of business profits, business interruption or other pecuniary loss) arising out of or inability to use this product.

All products from ERMA-Electronic are warranted against defective material and workmanship for a period of two (2) years from date of delivery. If it is necessary to return the product to ERMA, the sender is responsible for shipping charges, freight, insurance and proper packaging to prevent breakage in transit. ERMA's warranty does not apply to defects resulting from action of the buyer, such as mishandling, improper interfacing, operation outside of design limits, improper repair or unauthorized modification.

Warenzeichen

All trademarks are the property of their respective owners. ERMA-Electronic and its suppliers do not warrant the accuracy or completeness of the information provided herein. ERMA-Electronic and its suppliers do not warrant the accuracy or completeness of the information provided herein. ERMA-Electronic and its suppliers do not warrant the accuracy or completeness of the information provided herein.

CONTENTS

1. Description	4
2. Safety instructions	5
2.1. Explanation of symbols	5
3. Mounting	6
3.1. Place of operation	6
3.2. Panel mounting	6
3.2.1. Panel for switch board	6
3.2.2. Panel for mosaic systems	7
4. Electrical connections	8
4.1. General instructions	8
4.2. Hints against noisy environment	8
4.3. Connection and pin assignment	9
4.4. Connection of serial input signals	10
4.4.1. Connection of RS 232-signals for MT 2611	10
4.4.2. Connection of RS 485-signals for MT 2612	10
4.4.3. Connection of Current Loop signals for MT 2613	10
4.5. Digital inputs	10
4.6. Connection of the optocoupler	11
4.7. Connection of power supply voltage	11
5. Start-Up	12

6. Procedure of programming	13
6.1. Summary of the programming level	15
6.2. Programming level for configuration P-00	16
6.3. Programming level of alarm P-03	17
6.3.1. Alarm high setpoint	18
6.3.2. Alarm low setpoint	18
6.4. Programming quick reference	20
7. Utilization of the serial interface	20
7.1. Data format	20
7.2. Transfer characteristic	20
8. Software functions	22
8.1. Display test	22
9. Technical Specifications	22
10. Ordering Information	23
11. Supplement A - ASCII-table	24
12. Notices	25

Stand : 16.09.03
MT261XAE.PUB
Subjects to technical modifications

1. Description

The digital panel meters **MT 2701**, **MT 2702** and **MT 2703** are universal instruments for displaying serial transmitted ASCII-Codes.

Following interfaces are available:

MT 2701:	RS 232 signal input
MT 2702:	RS 485 signal input
MT 2703:	TTY (Current Loop, 20 mA) signal input

Following characters can be displayed:

- -, 0, 1, 2, 3, 4, 5, 6, 7, 8, 9, A, B, C, D, E, F
- blank, decimal point
- “+” is shown as a blank

Standard hardware

- Three digital inputs
- Optocouple output for limiting value indication

Standard software

- Programmable baud rate (1200, 2400, 4800, 9600 Baud)
- 3 selectable address characters
- Possibility to mask out max. 127 characters
- Display test

2. Safety instructions

This instrument is produced in accordance with Class II of IEC 348 and VDE 0411. When delivered the instrument has been tested to meet all functions described. Before installing the instrument please read the mounting and servicing instructions.

We have no liability or responsibility to customer or any other person or entity with respect to any liability, loss or damage caused or alleged to be caused directly or indirectly by equipment or software sold or furnished by us. Read the installation instruction carefully. No liability will be assumed for any damage caused by improper installation.

Inspect the instrument module carton for obvious damage. Be shure there are no shipping and handing damages on the module before processing. Do not apply power to the instrument if it has been damaged.

ERMA's warranty does not apply to defects resulting from action of the buyer, such as mishandling, improper interfacing, operation outside of design limits, improper repair or unauthorized modifications.

2.1. Explanation of symbols



Caution



Attention



Instruction



Hint

Caution: **Dangerous!**

Attention: Will cause **damage**.

Instruction: If not noticed, **trouble** may occur.

Hint: Useful hints for **better operation**.

3. Mounting


3.1. Place of operation

Attention must be paid to the protection against humidity, dust and high temperatures at the place of operation.

3.2. Panel mounting


3.2.1. Panel for switch board

- For mounting in switch boards, insert the case into the panel cutout (according to DIN 43700: $92,0^{+0,8} \times 22,2^{+0,6}$ mm) from the front, using a fresh gasket for sealing as required. Click into and place at each side the two fastening clips (M2,5 x 50 mm).
- Tighten the screws alternately, using enough pressure to get good retention and sealing at the panel.


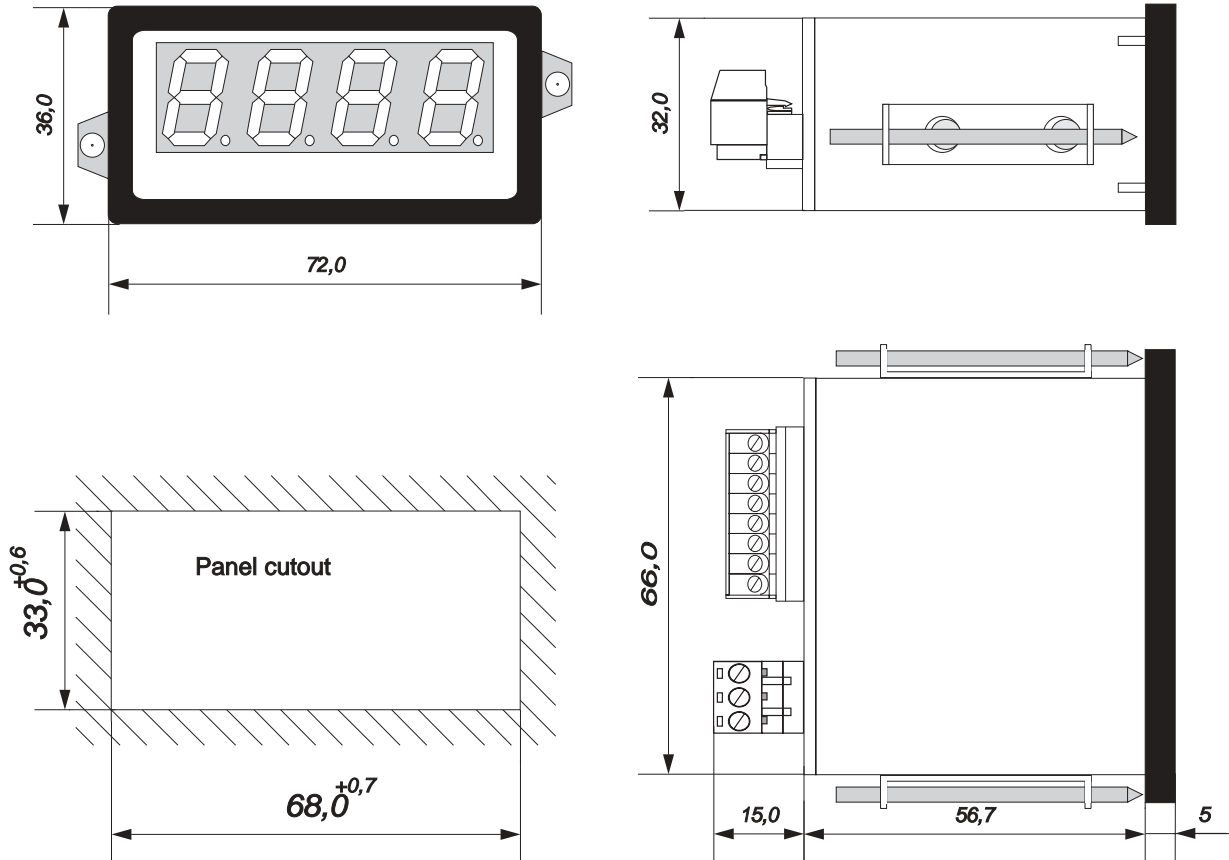


3.2.2. Panel for mosaic systems

- Insert the case into one of the following mosaic-systems:
 - a) Mosaic-system 8RU (M50x25) from Siemens
 - b) Mosaic-system from Subkleb

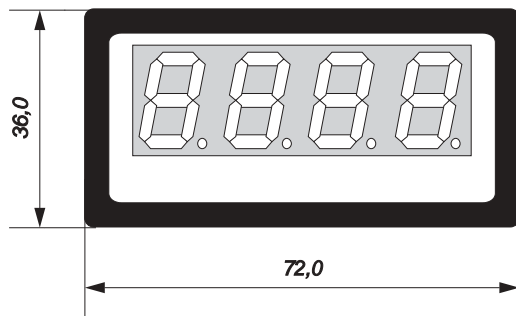

Mosaic system:
Siemens 8RU (M50x25)

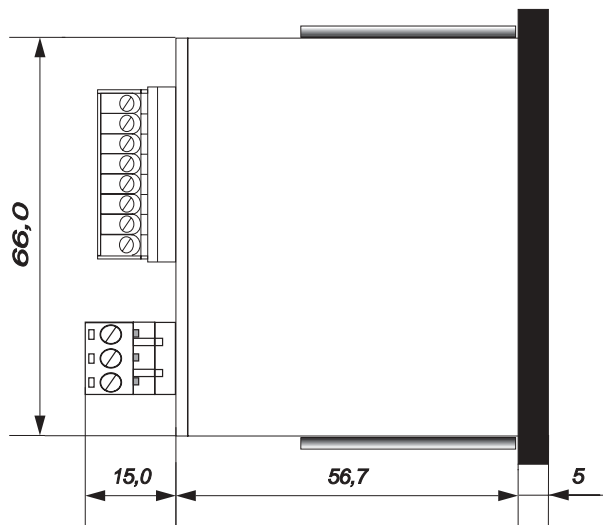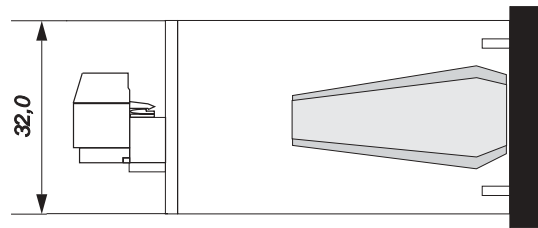

4. *Electrical connections*

4.1. *General instructions*



- It is forbidden to plug or unplug connectors with voltage applied
- Attach input and output wires to the connectors only without voltages applied
- Cords must be provided with sleeves
- Attention must be paid that the power supply voltage applied will agree with voltage noticed at the name plate.
- The instrument has no power-on switch, so it will be in operation as soon as the power is connected.

4.2. *Hints against noisy environment*

All inputs and outputs are protected against noisy environment and high voltage spikes. Nevertheless the location should be selected to ensure that no capacitive or inductive interference can have an effect on the instrument or the connection lines.


It is advisable:



- To use shielded cables.
- The wiring of shields and ground (0V) should be star-shaped.
- The distance to interference sources should be as long as possible. If necessary, protective screen or metal enclosures must be provided.
- Coils of relays must be supplied with filters.
- Parallel wiring of input signals and AC power lines should be avoided.

4.3. Connection and pin assignment

All inputs and outputs are connectors, designed as plug-in screw terminals.

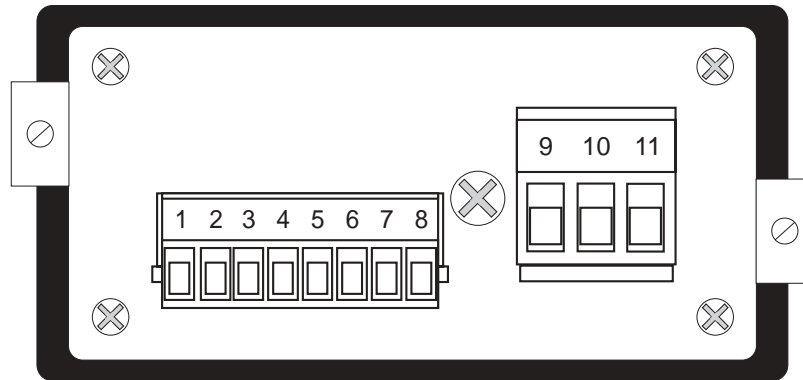


Pin assignment:


1	optocoupler output (emitter)	9	ground
2	optocoupler output (collector)	10	supply voltage (-)
3	digital input 1/display test	11	supply voltage (+)
4	digital input 2	12	
5	digital input 3	13	
6	MT 2701: n.c. MT 2702: RS 485-input, A(+) MT 2703: n.c.	14	
7	MT 2701: RS 232-input TxD MT 2702: RS 485-input, B(-) MT 2703: TTY-signal (+)	15	
8	MT 2701: RS 232-input GND MT 2702: RS 485-input GND MT 2703: TTY-signal (-)		

4.4. Connection of serial input signals


4.4.1. Connection of RS 232-signals for MT 2701

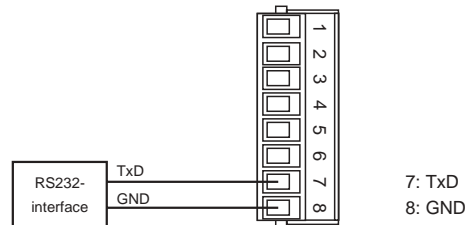


4.4.2. Connection of RS 485-signals for MT 2702

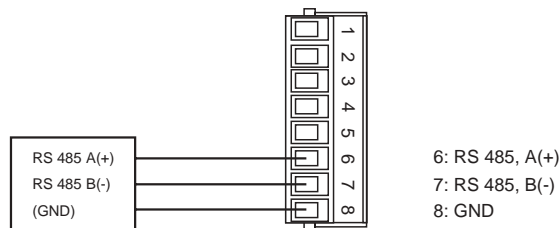

4.4.3. Connection of Current Loop signals for MT 2703

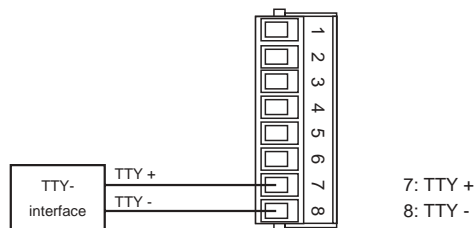

4.5. Digital inputs

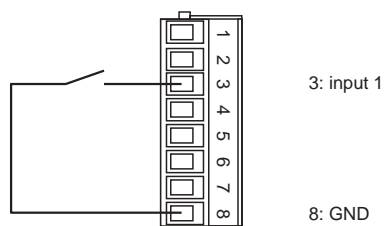

Digital input 1

- active => connecting screw terminal 3 to 8
- connecting to ground, low-active


Digital input 2

- active => connecting screw terminal 4 to 8
- connecting to ground, low-active


Digital input 3

- active => connecting screw terminal 5 to 8
- connecting to ground, low-active

4.6. Connection of the optocoupler

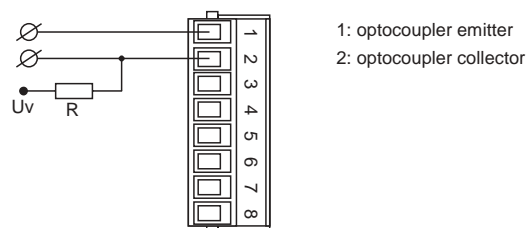

4.7. Connection of power supply voltage

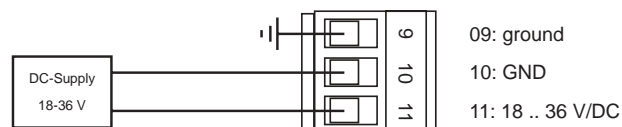

5. Start-Up



Attention must be paid that the power supply voltage applied will agree with the voltage noticed at the name plate.

Switch the power supply on (supply voltage applied to 10 (-) and 11 (+)).


When delivered, the instrument is programmed with a standard configuration (default configuration). According to his measuring task, the customer can change the standard configuration by programming.



Attention: When the instrument is built-in a machine and the customer wants to change the configuration, attention must be paid, that no damage will occur to the machine!

6. Procedure of programming

The procedure of programming is organized in different steps and can be carried out via the screw terminals 3, 4 and 5 at the rear of the instrument. It is advisable to connect a push button to the screw terminals 3 - 5.

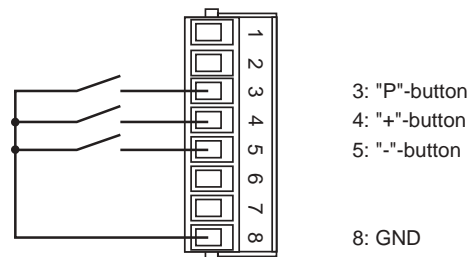

Push Button	Pressing
screw terminal 3 "P" - button	selection of - programming level - parameter
screw terminal 4 "+" - button	increase of - programming level - number of parameter - parameter
screw terminal 5 "- " - button	decrease of - programming level - number of parameter - parameter

Activating the programming routine

- Press "P"-button together with "+"-button
- The display shows "P-00"

Leaving the programming routine

- Press “+”-button or “-”-button until the display shows “PEnd”
- Confirm the display “PEnd” by pressing “P”-button
- Return to normal measuring

Selection of a programming level

- Selecting a programming level by pressing the “+”-button or “-”-button
- Confirm the selected programming level by pressing the “P”-button
- The display shows the parameter number of the selected programming level
e.g.: “0-00” => Parameter 0 of programming level 0
e.g.: ”3-00” => Parameter 0 of programming level 3

Leaving a programming level

- Press “+”-button or “-”-button until the display shows “xEnd”
e.g.: “0End” =>leaving programming level 0
e.g.: “3End” =>leaving programming level 3
- Confirm the display “xEnd” by pressing “P”-button
- The display shows the programming level
e.g. “P-00” => programming level 0
e.g. ”P-03” => programming level 3

Selection of a parameter

- Selection the parameter by pressing “+”-button or “-”-button
- Confirm the parameter by pressing “P”-button
- The display shows the last programmed value of the selected parameter

Change and confirm a selected parameter

- Change the parameter by pressing the “+”-button or “-”-button
- Confirm the parameter by pressing “P”-button

The display shows the programming level and the number of the parameter
e.g.: “0-05” => Parameter 5 of programming level 0
e.g.: ”3-03” => Parameter 3 of programming level 3

6.1. Summary of the programming level

The parameters of the panel meter are organized in different programming levels.

P-00: Programming level for general configuration of the panel meter

This level is used to adapt the panel meter and the serial interface.

P-03: Programming level for the alarm configuration

All settings for the alarm can be changed in this programming level.

6.2. Programming level for configuration P-00

Param.	Description	Range	Default Value
0-00	Reserve: no function	-	-
0-01	Reserve: no function	-	-
0-02	Selection of baud rate: 0 -> 9600 Baud 1 -> 4800 Baud 2 -> 2400 Baud 3 -> 1200 Baud	0 .. 3	0
0-03	Brightness of the display 0 -> Brightness 50 % 1 -> Brightness 100 %	0 .. 1	1
0-04	1.address character, decimal selectable	1 .. 127	2
0-05	2.address character, decimal selectable	0 .. 127	48
0-06	3.address character, decimal selectable	0 .. 127	49
0-07	Number of characters to mask out	0 .. 127	0
0-08	Reserve: no function	-	-
0-09	Reserve: no function	-	-
0End	Leaving programming level P-00		


6.3. Programming level of alarm P-03

Param.	Description	Range	Default Value
3-00	Configuration of alarm 0 -> optocoupler as alarm off 1 -> optocoupler active by high limit 2 -> optocoupler active by low limit	0 .. 2	0
3-01	Alarm value	-9999 .. 99999	0
3-02	Alarm hysteresis	0 .. 99	0
3-03	Reserve: no function	-	-
3-04	Reserve: no function	-	-
3-05	Reserve: no function	-	-
3-06	Reserve: no function	-	-
3-07	Reserve: no function	-	-
3-08	Reserve: no function	-	-
3-09	Reserve: no function	-	-
3End	Leaving programming level P-03		




If other characters as -, 0, 1, 2, 3, 4, 5, 6, 7, 8, 9 are transmitted, the alarm value **must** be deactivated.


6.3.1. Alarm high setpoint

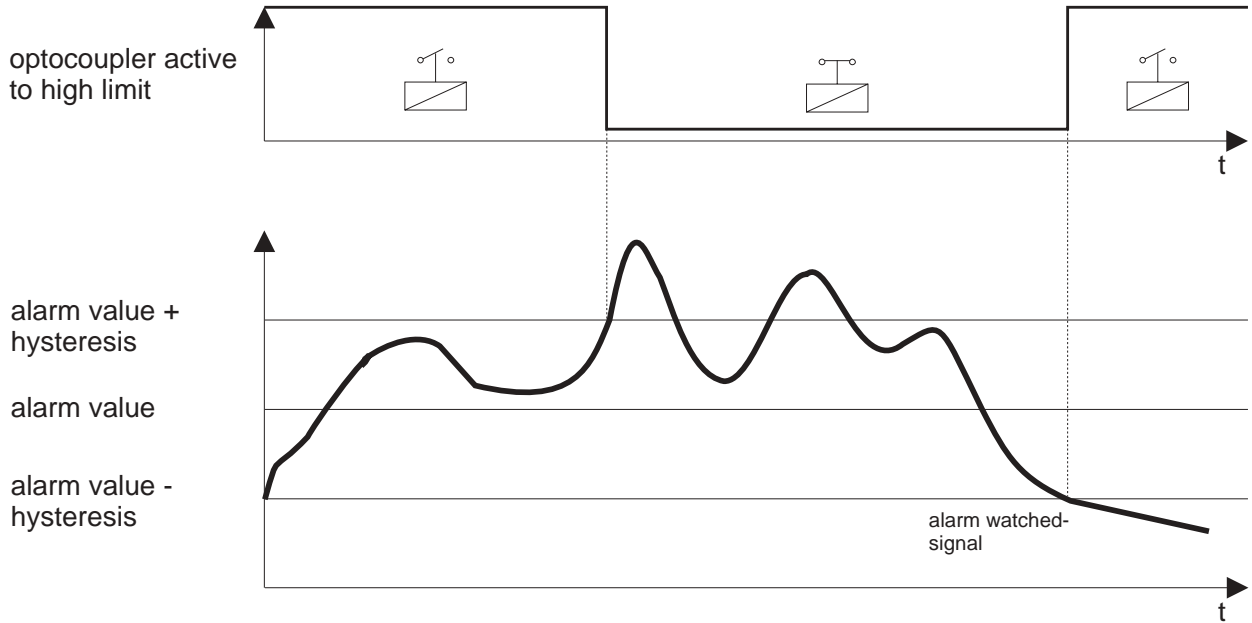

6.3.2. Alarm low setpoint

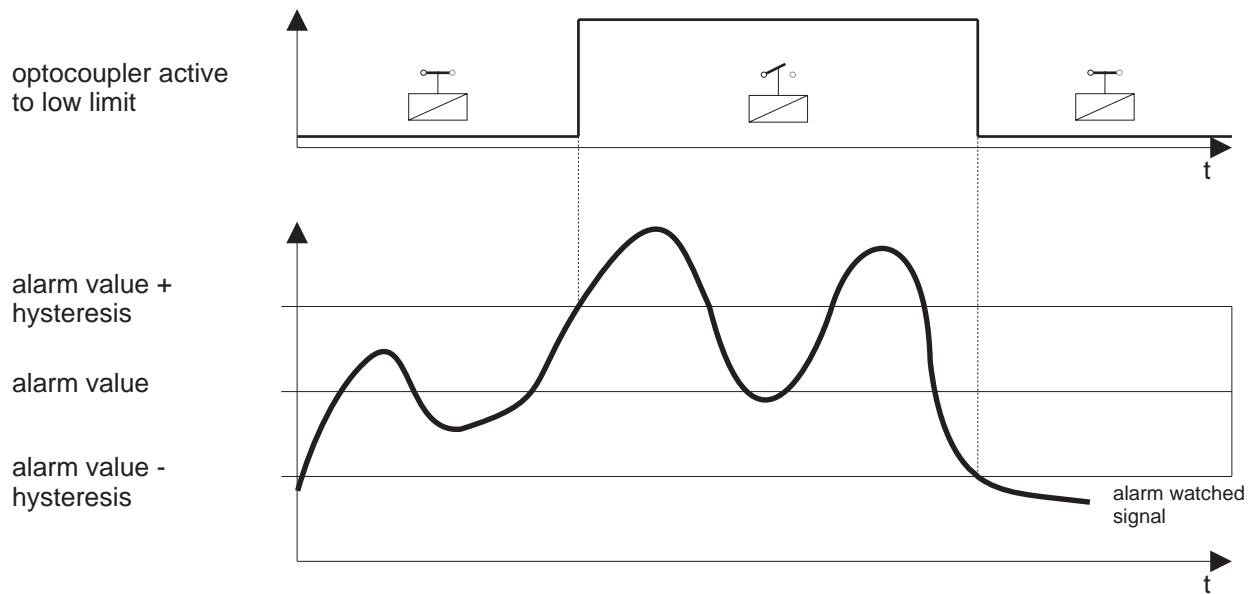

6.4. Programming quick reference

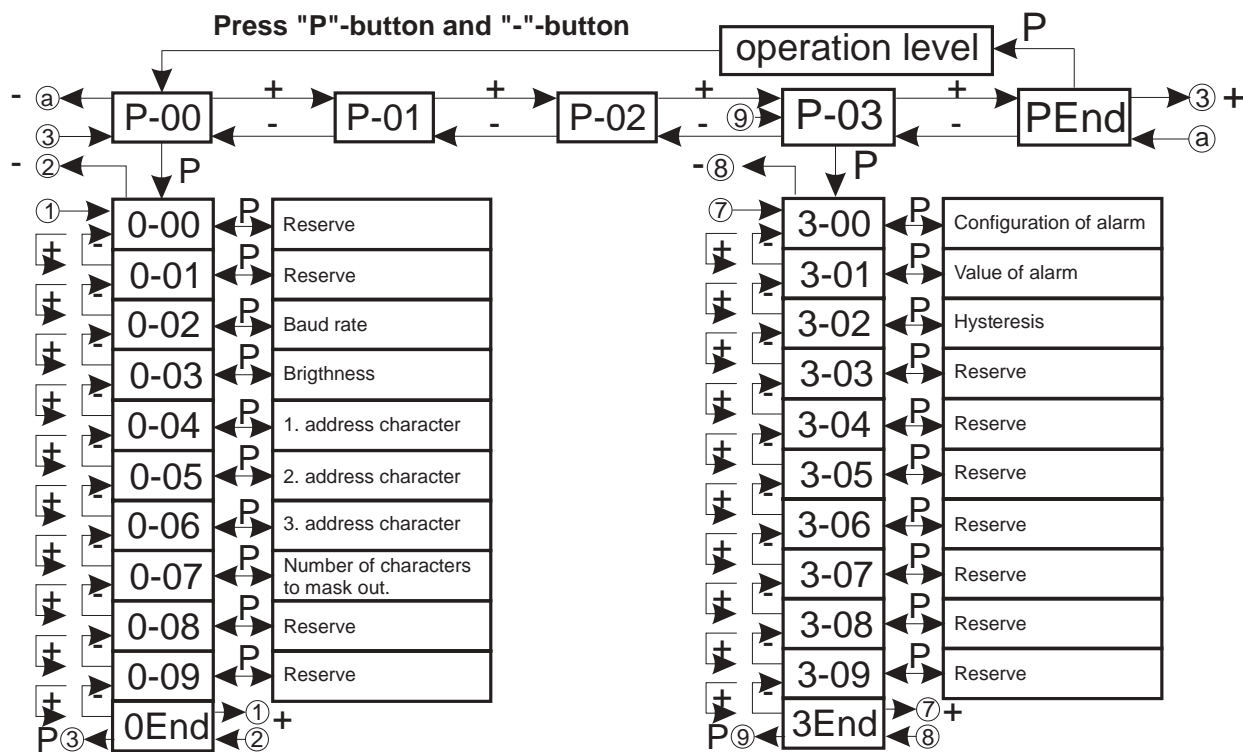

Description	
P	≡ pressing "P"-button (screw terminal 3)
+	≡ pressing "+"-button (screw terminal 4)
-	≡ pressing "-"-button (screw terminal 5)

7. Utilization of the serial interface

7.1. Data format

The format of transmission is built up as listed below:

1 Startbit	8 Databits	2 Stopbits
------------	------------	------------

The baud rate of the interface can be set in parameter 0-02. Following baud rates are available: 1200, 2400, 4800 or 9600 baud.

7.2. Transfer characteristic

Transmissions are built up as listed below:

AC1	AC2	AC3	Y .. Y	XXXXX
-----	-----	-----	--------	-------

List of characters:

AC1: First address character, decimal adjustable from 1 to 127

Recommended adjustment: 2_D (corresponding STX)

AC2: Second address character, decimal adjustable from 1 to 127

Recommended adjustment: 48_D - 57_D a. 65_D - 70_D (corr. 0 - 9 a. A - F)

AC3: Third address character, decimal adjustable from 1 to 127

Recommended adjustment: 48_D - 57_D u. 65_D - 70_D (corr. 0 -9 u. A - F)

The first address character must be programmed. In addition the second and the third address character can be programmed. Setting the corresponding parameters to 0, the second and the third address character are deactivated.

Y..Y: Number of characters which can be masked out, adjustable from 0 to 127.

The 5 characters following the last address character will be displayed. There can be a maximum of 127 other characters between the address characters and the real characters that will be displayed.

7. Utilization of the serial interface

XXXXX: Characters which will be displayed
(only following characters are approved)
-, 0, 1, 2, 3, 4, 5, 6, 7, 8, 9,
A, B, C, D, E, F
blank, decimal point
“+” is shown as a blank



In addition to the 5 characters, one decimal point can be displayed.

Example:

The signal sequence 123.5F of the following transmission should be displayed.

The transmission is built up as listed below:

“<STX>Temperature is 123.5F”

The **address characters** are STX, T and e.

Decimal values:

	ASCII-character	Decimal value
Parameter 0-04	STX	2
Parameter 0-05	T	84
Parameter 0-06	e	101

The number of characters that are masked out is 13.

The parameter 0-07 have to be programmed with 13.

By starting the transmission, **123.5F** will be displayed.

8. Software functions

8.1. Display test

When activating the display test all segments of the display are light on. The display shows "8.8.8.8.8."

Activating the display test:

- By activating the digital input 1, connecting screw terminal 3 and 8

9. Technical Specifications

Display range	: 4 characters
Communications protocol	: 1 start bit, 8 data bits, 2 stop bits 1200, 2400, 4800 or 9600 Baud
Input	
MT 2611	: RS 232
MT 2612	: RS 485
MT 2613	: TTY, (Current Loop, 20mA)
Digitale inputs	: 10 k Ω pull-up +5 V
Low-level	: < 0,4 V
High-level	: > 3,5 V, max. 30 V
Display	: 4 decades, 14 mm, red
optional	: green
Power supply	: 18 to 36 V DC (isolated)
power consumption	: max. 65 mA (red display) : max. 75 mA (green display)
optional	: 12 V DC, \pm 10 % (isolated) : 5 V DC, \pm 10 % (isolated)
Alarm contact	
Collector-Emitter-range	: max. 10 mA, 70 V, max. 150 mW
Case	: 96 x 24 x 63,5 mm
depth	: < 72 mm (incl. plug-in screw terminal)
protection case, at the front	: IP 40
protection case, connection	: IP 20
EMC	: in conform with 89/336/EWG
Operating temperature	: 0 bis 50 °C

10. Ordering Information

MT 270X -					
					Case 0 Panel mounting 1 Panel-clip
					Front becel color 0 Black
					Front design 0 Without front foil 1 Front foil ERMA-METER 2 Front foil NEUTRAL
					Display color 0 Red 1 Green
					Power supply 0 5 V DC, ± 10 % (isolated) 1 12 V DC, ± 10 % (isolated) 2 18 to 36 V DC (isolated)



Pay attention to the ordering number. Please order MT 2701, MT 2702 or MT 2703. (Dependent on the signal input)

11. Supplement A - ASCII-table

Dec.	Charac.	Dec.	Charac.	Dec.	Charac.	Dec.	Charac.
0	NUL	32	SP	64	@	96	`
1	SOH	33	!	65	A	97	a
2	STX	34	"	66	B	98	b
3	ETX	35	#	67	C	99	c
4	EOT	36	\$	68	D	100	d
5	ENQ	37	%	69	E	101	e
6	ACK	38	&	70	F	102	f
7	BEL	39	'	71	G	103	g
8	BS	40	(72	H	104	h
9	HT	41)	73	I	105	i
10	LF	42	*	74	J	106	j
11	VT	43	+	75	K	107	k
12	FF	44	,	76	L	108	l
13	CR	45	-	77	M	109	m
14	SO	46	.	78	N	110	n
15	SI	47	/	79	O	111	o
16	DLE	48	0	80	P	112	p
17	DC1	49	1	81	Q	113	q
18	DC2	50	2	82	R	114	r
19	DC3	51	3	83	S	115	s
20	DC4	52	4	84	T	116	t
21	NAK	53	5	85	U	117	u
22	SYN	54	6	86	V	118	v
23	ETB	55	7	87	W	119	w
24	CAN	56	8	88	X	120	x
25	EM	57	9	89	Y	121	y
26	SUB	58	:	90	Z	122	z
27	ESC	59	;	91	[123	{
28	FS	60	<	92	\	124	
29	GS	61	=	93]	125	}
30	RS	62	>	94	^	126	~
31	US	63	?	95	_	127	(DEL)

12. Notices

ERMA - Electronic GmbH
Max-Eyth-Straße 8
78194 Immendingen

Phone +49 7462 2000-0
Fax +49 7462 2000-29
Email info@erma-electronic.com
Web www.erma-electronic.com

ERMA

Electronic GmbH